

2009/09



LOT

2009/06

2015/09



Medical Device Class 1

Andropenis® Gold

1 unit - 1 unidad

Medical device for penis enlargement, correction of penile curvatures and urological post-surgical treatments / *Producto sanitario para alargamiento del pene, corrección de curvaturas peneanas y tratamientos post-quirúrgicos urológicos*

FOR PERSONAL USE ONLY – SUITABLE FOR PEOPLE ALLERGIC TO NICKEL
PARA USO INDIVIDUAL – APTO PARA ALÉRGICOS AL NÍQUEL

Read instructions before using the product / *Lea las instrucciones antes de usar el producto*

Store in cool and dry conditions. Non-sterile product.
Conservar en un lugar fresco y seco. Producto no estéril.

Made in Spain by / Fabricado en España por: ANDROMEDICAL, S.L.
c/ Proción, 7. E-28023 Madrid (Madrid), SPAIN
www.andromedical.com — email: support@andromedical.com




Component of Andropenis®. FOR PERSONAL USE ONLY
Componente de Andropenis®. PARA USO INDIVIDUAL
Made in Spain by / Fabricado en España por: ANDROMEDICAL, S.L.



MEDIUM ROD 2 cm



SMALL ROD 0,5 cm



SPRINGS




Protective Silicone Ring
Anillo protector de silicona

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Androsilicone®

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Androsilicone®

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01

2010/04



LOT

2010/01

2020/01



Medical Device Class I

Andropenis® Gold

1 unit - 1 unidad

Medical device for penis enlargement, correction of penile curvatures and urological post-surgical treatments / *Producto sanitario para alargamiento del pene, corrección de curvaturas peneanas y tratamientos post-quirúrgicos urológicos*

FOR PERSONAL USE ONLY – SUITABLE FOR PEOPLE ALLERGIC TO NICKEL
PARA USO INDIVIDUAL – APTO PARA ALÉRGICOS AL NÍQUEL

Read instructions before using the product / *Lea las instrucciones antes de usar el producto*

Store in cool and dry conditions. Non sterile/non measuring product.
Conservar en un lugar fresco y seco. Producto no estéril/Sin función de medición.

Made in Spain by / Fabricado en España por: ANDROMEDICAL, S.L.
c/ Proción, 7. E-28023 Madrid (Madrid), SPAIN
www.andromedical.com — email: support@andromedical.com

After completing the treatment, please separate all plastic parts from metal parts and dispose of them in the appropriate recycling containers.
Tras finalizar el tratamiento, despiece el aparato y deposite por separado las partes de plástico y las partes de metal en los envases de reciclaje adecuados.




Comfort Kit®

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Premium Kit®

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Andropenis® for Androsilicone®

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Andropenis® for Andropenis® Band

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Androsilicone®

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Protective Silicone Ring (optional)
Anillo protector de silicona (opcional)

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01




Andropenis® Band

Caution: before assembling or disassembling, please look the color.
Atención: antes de montar o desmontar, revise el color.

2 units - 2 unidades

Store in cool and dry conditions.
Conservar en un lugar fresco y seco.

2010/01

Product and component labels redesigned and adapted to European Medical regulations

New indication added in the main label of the product for the proper recycling process of the device.
New labels for the Andropenis® components.

2009/09



No comfort silicone band
(Androcomfort® Band)

2010/04



2 NEW comfort silicone bands
(Androcomfort® Band)

2009/09



No comfort protective cushion
(Androtop® for Androcomfort® Band)

2010/04



2 NEW comfort protective cushions
(Androtop® for Androcomfort® Band)

2009/09



3 silicone bands (Androsilicone®)

2010/04



2 silicone bands (Androsilicone®)

2009/09



3 protective cushions
(Androtop®)

2010/04



2 protective cushions
(Androtop®)

2009/09




3 Protective silicone rings (Androring®)

2010/04



2 Protective silicone rings (Androring®)

2009/09

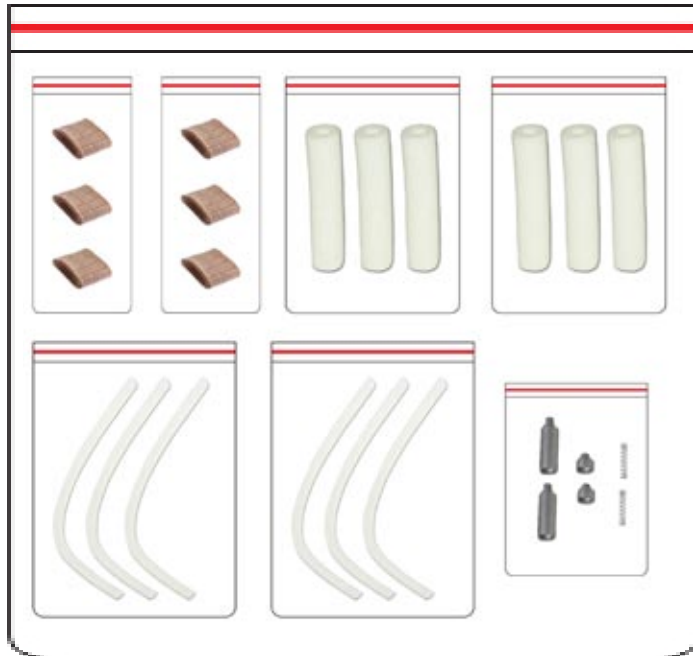

Premium Kit®
3 units per bag
(Androring®, Androtop®, Androsilicone®).

1 bag including all referred components.


2010/04



Premium Kit®
No quantity variation.
Only components redistributed.
2 units per bag;
additional bags included.
(Androring®, Androtop®, Androsilicone®)


1 bag including all referred components.

2009/09

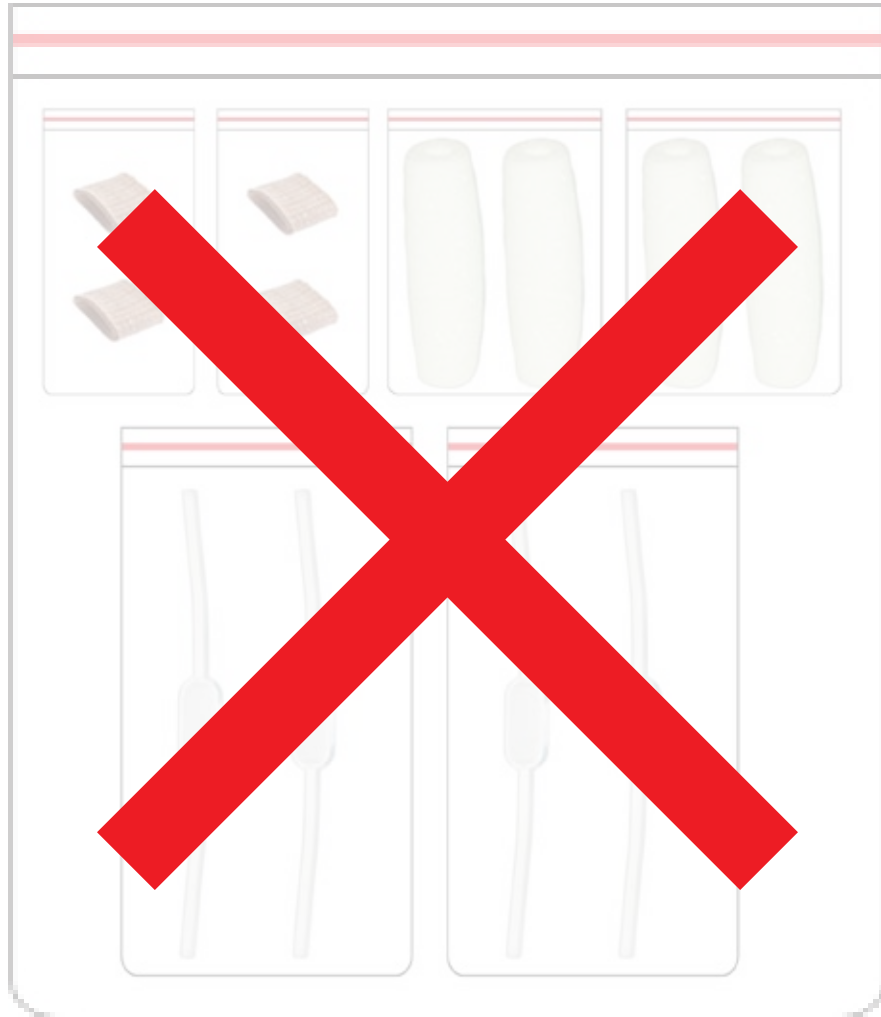

No Comfort Kit® available

2010/04

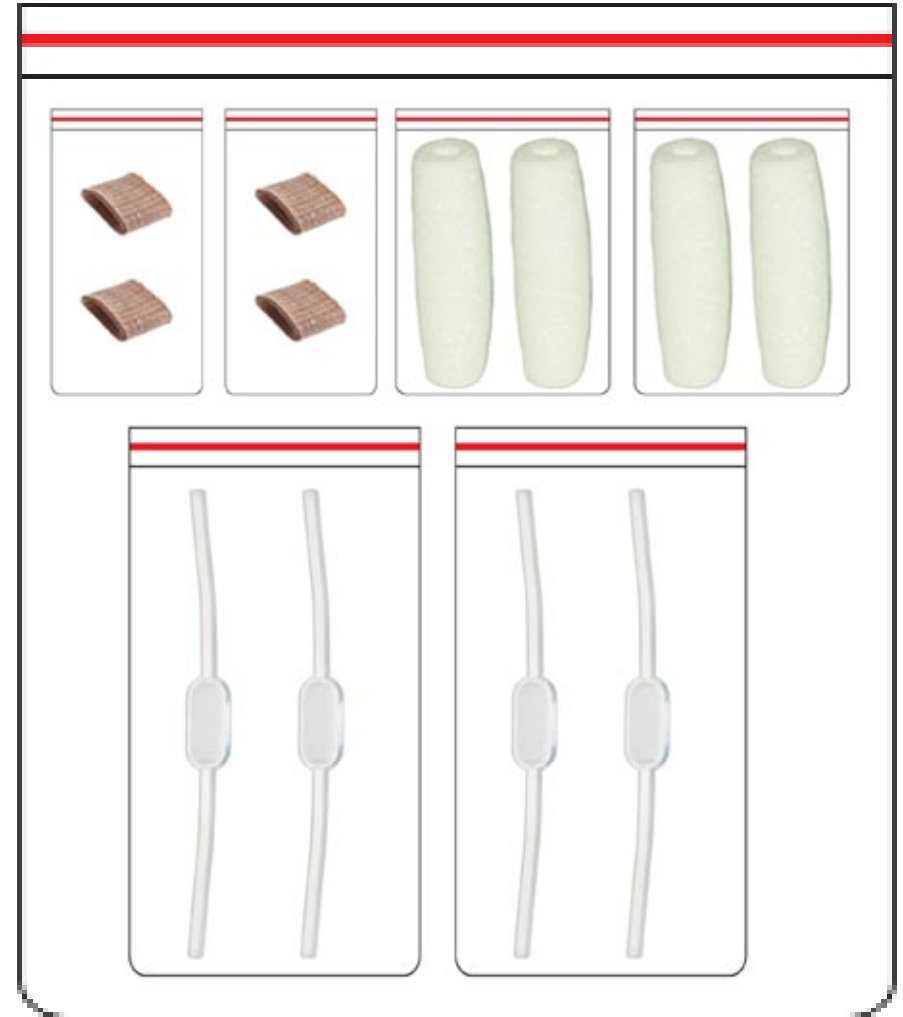

Comfort Kit® NOW available

2009/09




Instructions Manual

2010/04



Instructions Manual with the new
Androcomfort® Band mounted in the
Andropenis® Device

2009/09

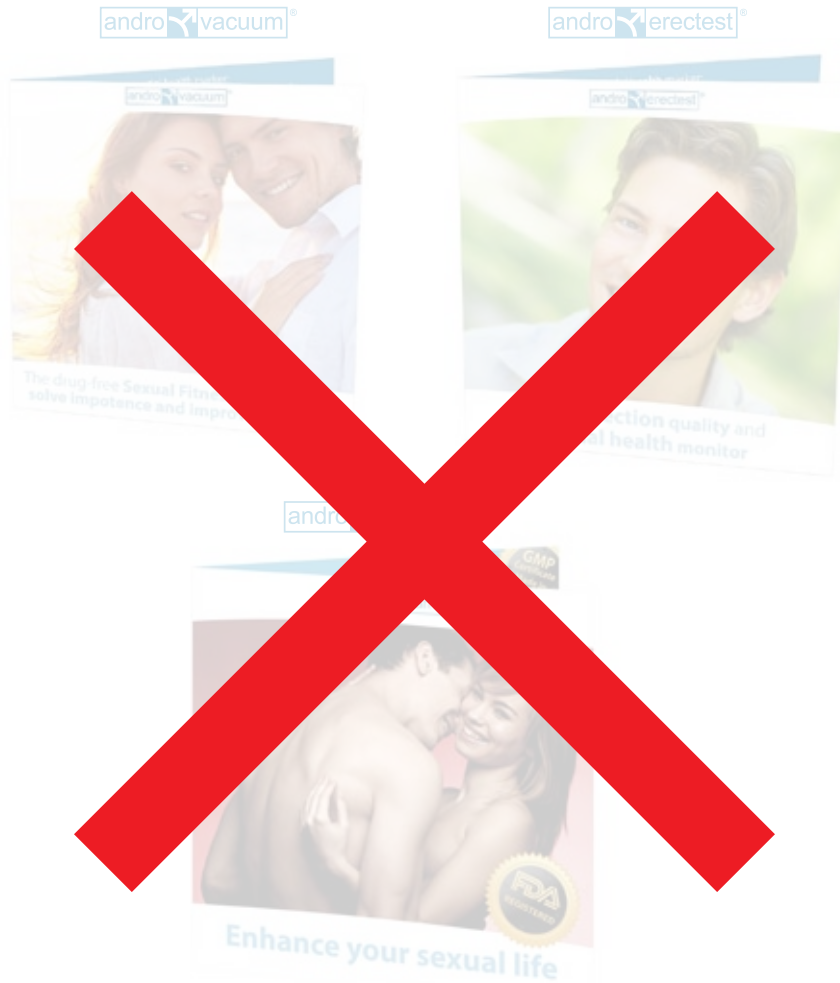

No Promotional Products inserts

2010/04



Promotional Products inserts

2009/09



Left side of the packaging

2010/04



Left side of the packaging with new sentence: "Read the instructions carefully before using the product"

2009/09



Front side of the packaging

2010/04



Front side of the packaging with a new Andropenis® picture, featuring the new Androcomfort® Band. Also added a new “Now in Gold” seal.

2009/09



Product presentation
with its components

2010/04



NEW product presentation
with its components